


-15kV TOF: -9181 v
 -3.6kV MCP: -3364 v
 -2.4kV MCP: -1774 v
 Input Cur: 310 ma
 RPA max: 237 v
 Mirror max: 238 v

Tue Oct 10 09:05:43 2006

TIDE Direct Events

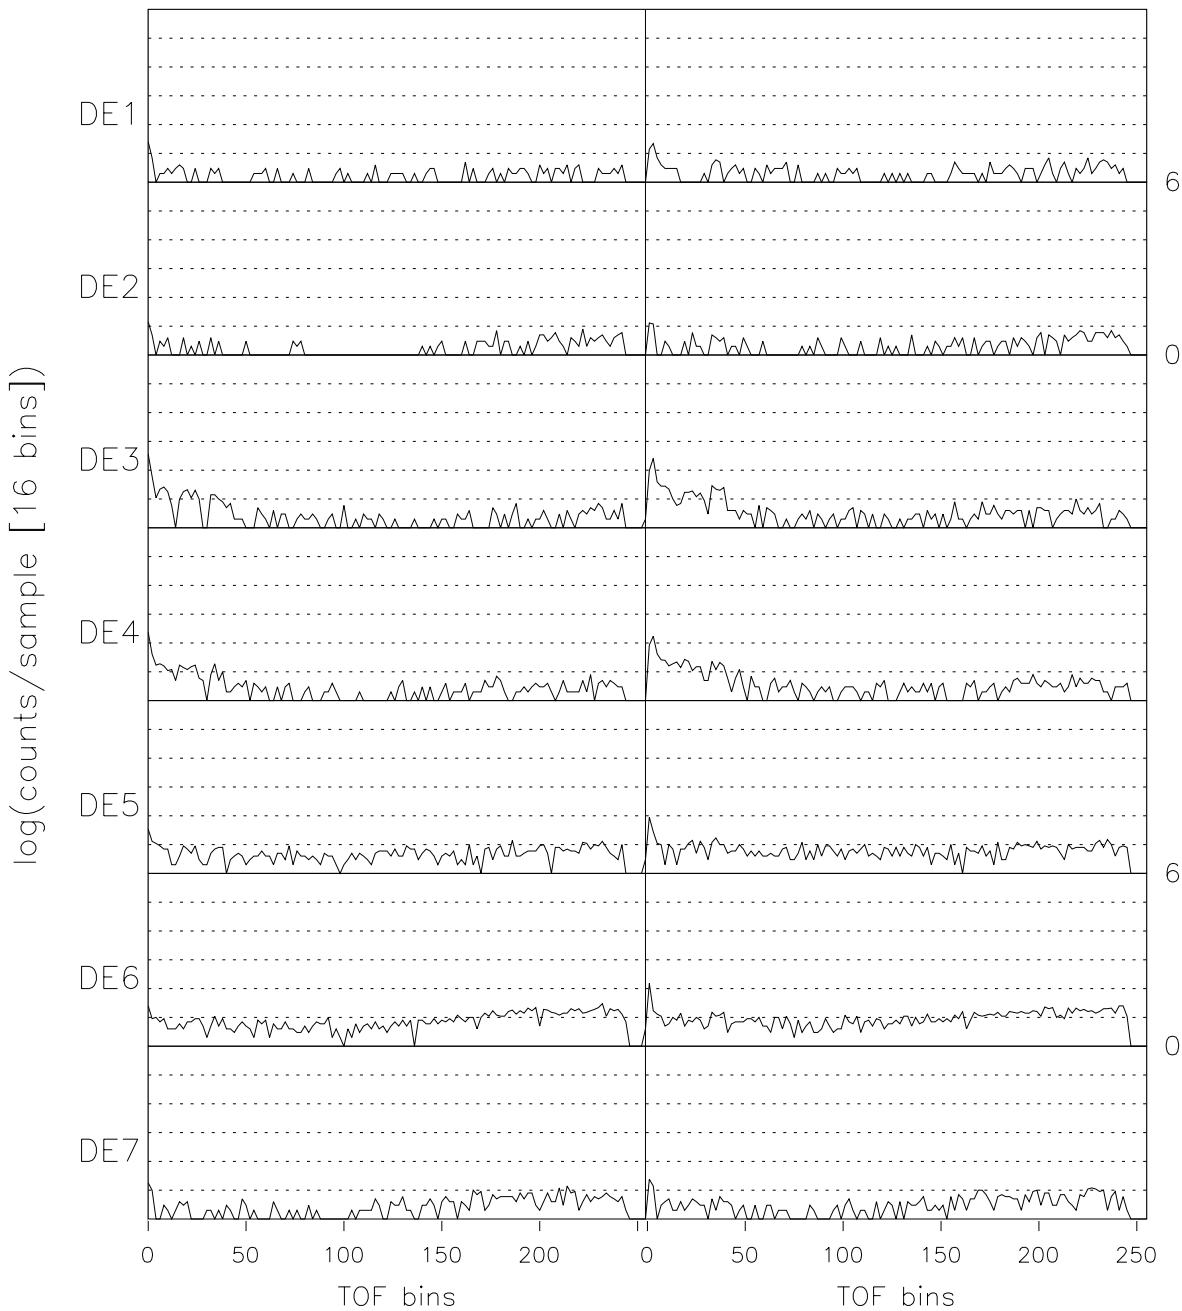

reported:

reported: 10-09-06 15:57:59 UT

file: /export/data/tide/nrt/nrt0610091554.lz

-15kV TOF: -9181 v

-3.6kV MCP: -3364 v

-2.4kV MCP: -1784 v

Input Cur: 318 ma

RPA max: 237 v

Mirror max: 238 v